


(VII) Streptococcus

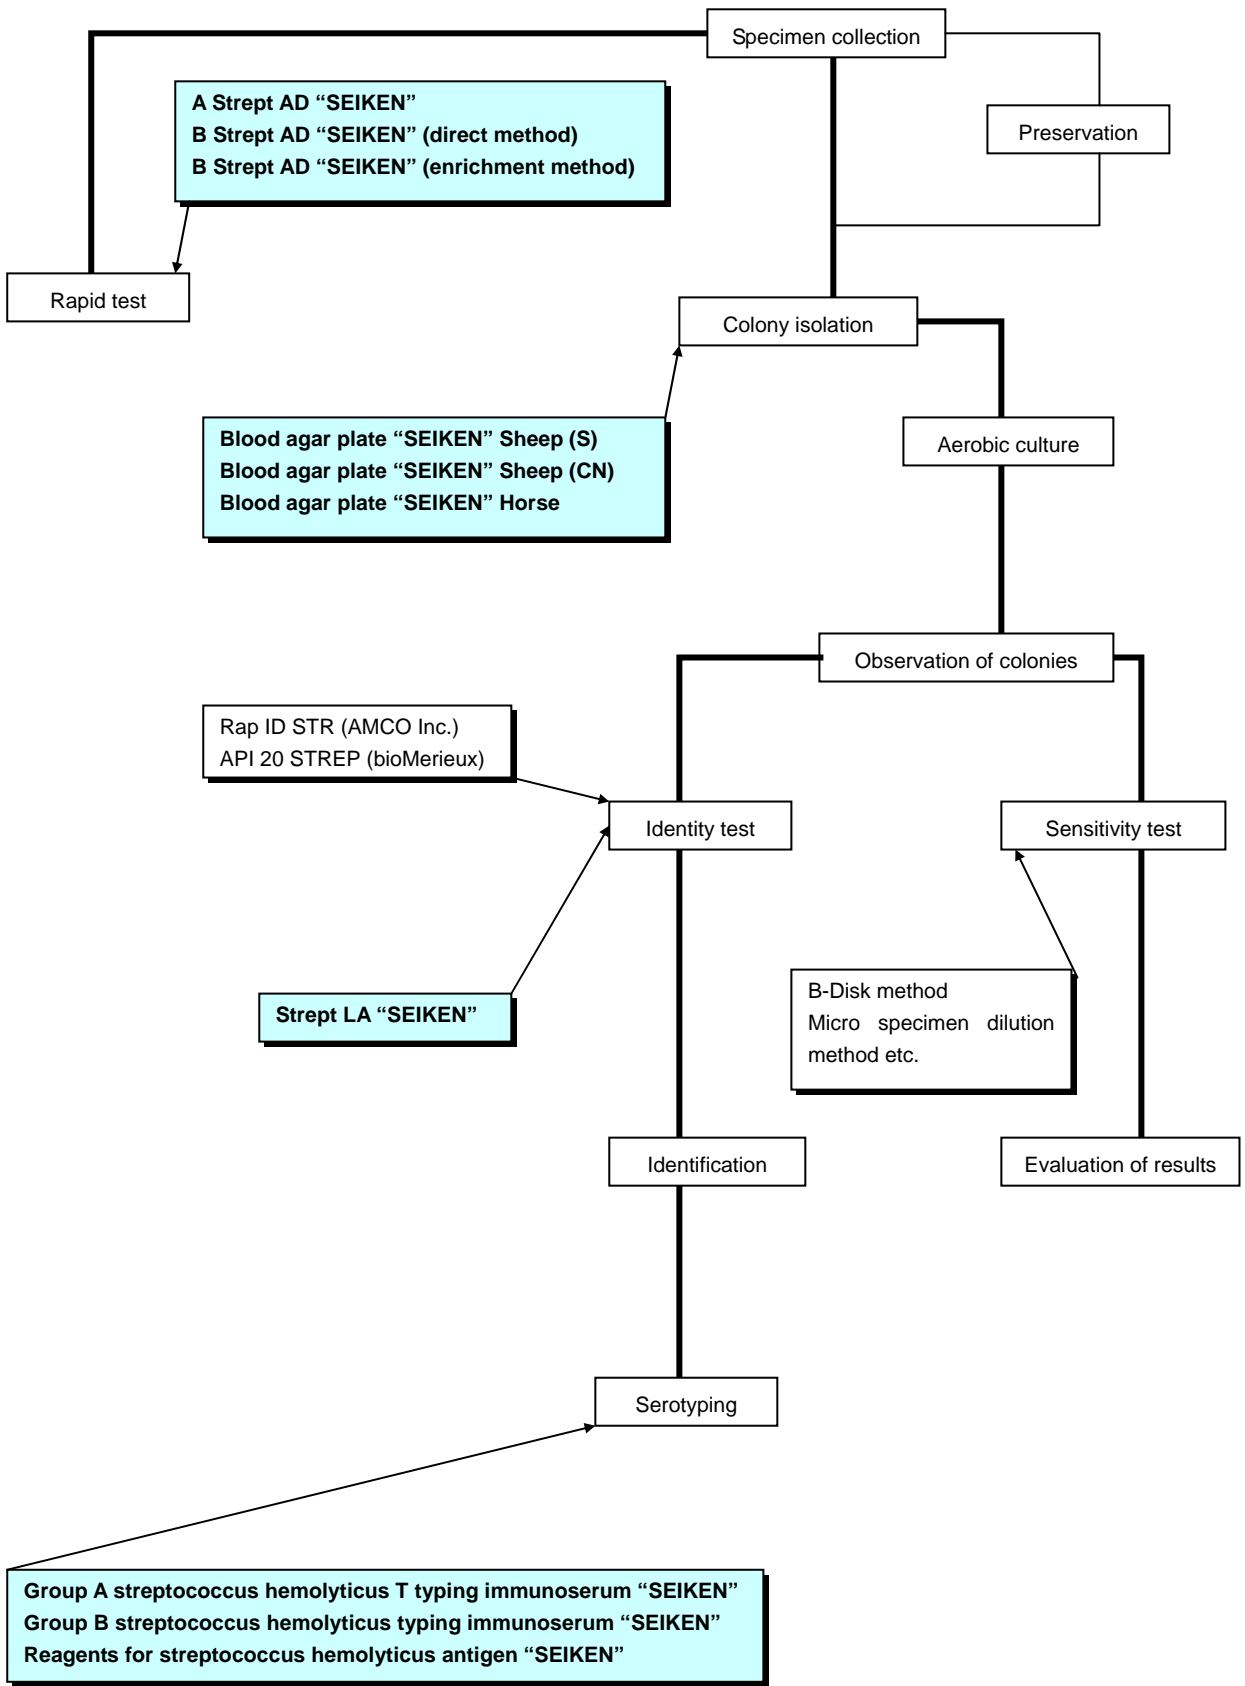

Group B is CE Marked

Streptococci Antisea					
Group-A T-Typing Set (2 mL x 24)			200327	Group-B Typing	
Polyvalent T	213235		Polyvalent X	213266	Set (2 ml x 6) 270023
T-1	213280		T-8	213341	Ia 270146
T-3	213303		T-14 / 49	213396	Ib 270153
T-13	213389		T-25	213433	II 270160
T-B3264	213457		T-Imp. 19	213464	III 270177
Polyvalent U	213242		Polyvalent Y	213273	IV 270184
T-2	213297		T-9	213358	V 270191
T-4	213310		T-18	213402	Also available
T-6	213334		T-22	213419	VI (NT6) 270207
T-28	213440		T-23	213426	VII (7271) 270221
Polyvalent W	213259		Auxiliary reagents		271013
T-5 / 27 / 44	213327		Pancreatic extract		
T-11	213365		pH adjustment		
T-12	213372		Phenol red		

Auxiliary Reagents for Typing of *Hemolytic Streptococcus*

Product Code 271013	Contents
<u>Kit contents</u>	
Swine pancreas extract	5 mL x 4 vials
pH correction solution	5 mL x 2 vials
Phenol red solution	5 mL x 1 vial

Strept-LA

Product Code 230201	Contents
Hemolytic Streptococci Grouping Kit by Slide Latex Agglutination	50 tests
<u>Kit contents:</u>	
Sensitized latex A	2 mL x 1 vial
Sensitized latex B	2 mL x 1 vial
Sensitized latex C	2 mL x 1 vial
Sensitized latex G	2 mL x 1 vial
Positive control	1 mL x 1 vial
Extraction reagent 1	5 mL x 1 vial
Extraction reagent 2	5 mL x 1 vial
Extraction reagent 3	5 mL x 1 vial
Test card	55 sheets
Sampling cup	55 pcs.
Pipette	55 pcs.
Mixing stick	220 pcs.

A Strept-AD “SEIKEN”

Product Code 230140	Contents
Group-A Streptococcal Antigen Detection Kit by Slide Latex Agglutination	50 tests
<u>Kit contents:</u>	
Sensitized latex	2 mL x 1 vial
Control latex	2 mL x 1 vial
Positive control	1 mL x 1 vial
Extraction reagent 1	5 mL x 1 vial
Extraction reagent 2	5 mL x 1 vial
Extraction reagent 3	5 mL x 1 vial
Sampling cup	55 pcs.
Pipette	55 pcs.
Sterile swab	55 pcs.
Test card	30 pcs.

B Strept-AD (Enrichment Detection Method)

Product Code 230522	Contents
Group-B Streptococcal Antigen Detection Kit by Slide Latex Agglutination	50 tests
<u>Kit contents:</u>	
Sensitized latex	2 mL x 1 vial
Control latex	2 mL x 1 vial
Positive control	1 mL x 1 vial
Extraction reagent 1	5 mL x 1 vial
Extraction reagent 2	5 mL x 1 vial
Extraction reagent 3	5 mL x 1 vial
Enrichment broth	3 mL x 1 vial
Sterile swab	50 pcs.
Test card	30 pcs.
Mixing stick	120 pcs.

B Strept-AD (Direct Detection Method)

Product Code 230515	Contents
Group-B Streptococcal Antigen Detection Kit by Slide Latex Agglutination	50 tests
<u>Kit contents:</u>	
Sensitized latex	2 mL x 1 vial
Control latex	2 mL x 1 vial
Positive control	1 mL x 1 vial
Extraction reagent 1	5 mL x 1 vial
Extraction reagent 2	5 mL x 1 vial
Extraction reagent 3	5 mL x 1 vial
Sampling cup	55 pcs.
Dropper	55 pcs.
Sterile swab	50 pcs.
Test card	30 pcs.
Mixing stick	120 pcs.

Streptococcus pneumoniae Antisera					
Set (2mL x 8 polyvalent, 39 monovalent)					270054
Polyvalent 1	270542	Polyvalent 4	270573	Polyvalent 7	270603
1	270627	17	270771	27	270863
2	270634	18	270788	32	270900
3	270641	21	270818	36	270948
4	270658	22	270825	38	270955
5	270665	Polyvalent 5	270580	39	270962
Polyvalent 2	270559	20	270801	Polyvalent 8	270610
6	270672	29	270887	7	270689
8	270696	31	270894	19	270795
9	270702	33	270917	24	270849
10	270719	34	270924	40	270979
Polyvalent 3	270566	35	270931		
11	270726	47	271006		
12	270733	Polyvalent 6	270597		
14	270740	23	270832		
15	270757	25	270856		
16	270764	28	270870		
		41	270986		
		46	270993		

All serotyping results by this kit were completely identical to those obtained by the conventional method.